



**All India Institute of Medical Sciences, Bhubaneswar**  
**At - Sijua (Patrapada), Post - Dumuduma, Bhubaneswar (Odisha) - 751 019**

To be uploaded in Website: [www.aiimsbhubaneswar.edu.in](http://www.aiimsbhubaneswar.edu.in) (Tender)

Reference No: **J-11057(011)/2017-18/S&P**

Dated: **21/02/2018**

**Sub: Purchase of Upper GI Endoscope (Adult) -150 Series & 190 Series as Proprietary basis-  
Inviting Comments thereon.**

The Department of Gastroenterology, AIIMS, Bhubaneswar has requested to purchase of **Upper GI Endoscope (Adult) -150 Series & 190 Series** from **M/s. Olympus Medical Systems India Private Limited, Haryana.**

The Notice is being uploaded for general information of prospective manufacturer/Authorized Distributor/Dealers to submit their objection/proposal/comments, if any, on proprietorship of the item.

In case the product of any manufacturer/Authorized distributor/Dealer conforms to the enclosed specifications, they may submit their proposal for the supply of the same along with the brochures, point by point compliance of the enclosed specifications along with all documentary evidence. One quotation of the product may also be submitted.

The objections/comments/proposal should be sent in sealed cover to the Office of Sr. Procurement Cum Stores Officer, AIIMS, Bhubaneswar (Odisha)-751019, so as to reach on or before **date:08-03-2018** falling which it will be presumed that no any other firm is interested to offer comments/protest/object and case will be decided on its merits.

The ref. no.-**J-11057(011)/2017-18/S&P** dt: **21-2-18**, due on date:08-03-2018 should be superscripted on sealed envelope.

**Enclosure:**

1. Proprietary Article Certificate from User Dept. of Gastroenterology, AIIMS, Bhubaneswar.

**Annexure-I**

2. Specification of required item. **Annexure-II**

3. Rate Certificate of M/s. Olympus Medical Systems India Private Limited, Haryana.

**Annexure-III**

4. Authorization Certificate of M/s. Olympus Medical Systems India Private Limited, Haryana.

**Annexure-IV**

5. CMC Charges submitted by M/s. Olympus Medical Systems India Private Limited, Haryana.

**Annexure-V**

6. PAC of M/s. Olympus Medical Systems India Private Limited, Haryana. **Annexure-VI**

7. Specification of M/s. Olympus Medical Systems India Private Limited, Haryana.

**Annexure-VII**

8. Quotations of M/s. Olympus Medical Systems India Private Limited, Haryana. **Annexure-VIII**

Copy to:

- |                                   |   |                              |
|-----------------------------------|---|------------------------------|
| 1. HOD, Dept. of Gastroenterology | : | for information Please.      |
| 2. Accounts Officer               | : | for information Please.      |
| 3. IT Cell                        | : | for hoisting in the website. |

  
**ए. के. दाश चौधुरी**  
**A. K. Dash Choudhury**  
**वरिष्ठ क्रय सह भण्डार अधिकारी**  
**Sr. Procurement-cum-Stores Officer**  
**एम्स भुवनेश्वर - 751019**  
**AIIMS, Bhubaneswar - 751019**

ANNEXURE  
Documents  
Upper GI

ANNEXURE - I

## Proprietary Article Certificate

Valid for the Current Financial Year

②

|                                                                                    |                                                                                                                                                                                                                                                          |                                  |                                            |
|------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------|--------------------------------------------|
| <b>File No. and Date Reference :</b>                                               |                                                                                                                                                                                                                                                          |                                  |                                            |
| 1                                                                                  | Description of article                                                                                                                                                                                                                                   | Upper GI Endoscope - 190 series  |                                            |
| 2                                                                                  | Forecast of quantity /annual requirement                                                                                                                                                                                                                 | 01                               |                                            |
| 3                                                                                  | Approximate estimated value for above quantity                                                                                                                                                                                                           | Rs 18 Lakh                       |                                            |
| 4                                                                                  | Maker's name and address                                                                                                                                                                                                                                 | Olympus - Gurgaon                |                                            |
| 5                                                                                  | Name's of authorised dealers/ stockists                                                                                                                                                                                                                  | Olympus - Gurgaon                |                                            |
| 6                                                                                  | I approve the above purchase on PAC basis and certify that : -<br>Note- Tick to retain only one out of (b), C-1) or (c-2) whichever is applicable and cross out others.<br>Please do confirm (a) by ticking it- without PAC certificate will be invalid. |                                  |                                            |
| 6 (a)                                                                              | This is the only firm who is manufacturing / stocking this item.<br>AND                                                                                                                                                                                  |                                  | ✓                                          |
| 6 (b)                                                                              | A Similar article is not manufactured / sold by any other firm, which could be used in lieu                                                                                                                                                              |                                  | X                                          |
| 6 (c-1)                                                                            | No other make/brand will be suitable for following tangible reasons (like OEM/Warranty spares.) : OR<br>Because in the dept there is existing 190 series videoprocessor CCLV-190) (Olympus)                                                              |                                  | ✓                                          |
| 6 (c-2)                                                                            | No other make/brand will be suitable for following intangible reasons (if PAC was also given in the last procurement cycle, please also bring out efforts made since then to locate more sources) :                                                      |                                  | X                                          |
| 7                                                                                  | Reference of concurrence of finance wing to the proposal :                                                                                                                                                                                               |                                  |                                            |
| History of PAC Purchase of this item for past three years may be given below : N/A |                                                                                                                                                                                                                                                          |                                  |                                            |
| Name of the Supplier                                                               |                                                                                                                                                                                                                                                          |                                  |                                            |
| <b>Order/ Tender Reference &amp; Date</b>                                          | <b>Quantity Ordered</b>                                                                                                                                                                                                                                  | <b>Basic Rate on Order (Rs.)</b> | <b>Adverse Performance Reported if Any</b> |
|                                                                                    |                                                                                                                                                                                                                                                          |                                  |                                            |
|                                                                                    |                                                                                                                                                                                                                                                          |                                  |                                            |
|                                                                                    |                                                                                                                                                                                                                                                          |                                  |                                            |

Signature of the Indenter/ User

Signature of Approving Authority.....

Date..... Designation of Officer.....

Dr. Manas Kumar Panigrahi  
Assistant Professor  
Dept. of Gastroenterology  
AIIMS Bhubaneswar-751005

**4. Upper GI Endoscope Adult :- 01 (one)**

- Field of view : Normal and Near focus 140 degree or more
- Direction of view : 0 degree, forward viewing
- Depth of field : 2-6 mm near and 5-100 mm normal
- Distal end outer diameter : 9.9 mm or less
- Insertion tube outer diameter : 9.9 mm or less
- Tip bending range : Up 210 deg, Down 90 deg, Left & Right 100 deg.
- Working length : 1030 mm or more
- Channel inner diameter : 2.8 mm or more
- Should have HDTV compatible CCD with Near & Normal focus observation capacity
- Should be equipped with Auxiliary water jet for mucosal cleaning
- Fully immersible in disinfectant solution (no need to attach water resistant cap) & one touch connectivity.
- The endoscope should be compatible with a processor capable of optical chromo endoscopy
- It should provide high resolution vision.
- It must be latest and using high-end technology
- Standard accessories Standard accessories including
  - 8 Compatible oval biopsy forceps- 5 in number
  - 9 Reusable alligator biopsy forceps-5 in number
  - 10 Cleaning brush - 5 in number
  - 11 Extra suction and air water channel valves- 2 in number
  - 12 Biopsy valve- 10 packets
- **The endoscope must be compatible with our existing light source & video processor (190 series) which are available in the Endoscopy Suite, Department of Gastroenterology, AIIMS, Bhubaneswar.**
- Provide with latest compact high end computer (desktop with high storage capacity at least 1TB), with latest processor with original latest windows and fully installed original latest Microsoft office version (one time purchase & installation), antivirus

software with 3 year validity, endoscopy reporting software enabled, high end latest laser colour printer from reputed brand and UPS with 1 kv capacity (all units are of one each).

Terms and conditions:

- The system must have a standard comprehensive warranty of 5 years with spares and should quote CMC for next 5 years.
  - It should be certified that if the instrument becomes non functional, it will be repaired within the shortest possible time period otherwise a penal charge will be levied on the company.
  - The vender should have service centre in Bhubaneswar
-

**OLYMPUS®**

Your Vision, Our Future

**OLYMPUS MEDICAL SYSTEMS INDIA PRIVATE LIMITED.**  
Ground Floor, Tower-C, SAS Tower, The Medicity Complex,  
Sector - 38, Gurgaon 122001, Haryana, INDIA  
Tel. : 0124-4999191 Fax : 0124-4999190  
Website : [www.olympusmedical.co.in](http://www.olympusmedical.co.in)  
CIN : U33110HR2009FTC039611

Date: 19.02.2018

To,  
The Director  
All India Institute of Medical Sciences,  
Bhubaneswar

Ref: - Mail Dtd 10-02-2018 regarding the purchase on PAC


Sub: Rate Certificate.

Dear Sir,

We Olympus Medical Systems India Pvt. Ltd. Gurgaon do hereby confirm that the rates offered against the above reference number are reasonable and justified and are not marketing lower rates to other Institutions on the same conditions of the bid and contract.

Yours sincerely  
For Olympus Medical Systems India Pvt. Ltd.

1/7  
Authorised Signatory



**OLYMPUS**

Your Vision, Our Future

**OLYMPUS CORPORATION****Headquarters**Shinjuku Monolith, 3-1 Nishi-Shinjuku 2-chome, Shinjuku-ku,  
Tokyo 163-0914 Japan**Technology Research Institutes**2951 Ishikawa-machi, Hachioji-shi, Tokyo 192-8507 Japan  
2-3 Kuboyama-cho, Hachioji-shi, Tokyo 192-8512 Japan**Dated: 7<sup>th</sup> March 2017****TO WHOMSOEVER IT MAY CONCERN****Sub.: Authorization letter**

Dear Sir,



We, **Olympus Corporation** having our office at Shinjuku Monolith, 3-1 Nishi-Shinjuku 2 – Chome, Shinjuku-ku, Tokyo 163-0914, Japan, do hereby confirm that **Olympus Medical Systems India Private Limited** having their registered office at Ground Floor, Tower-C, SAS Tower, The Medicity Complex, Sector- 38, Gurgaon-122001, Haryana, India, is 100% subsidiary of **Olympus Corporation of Asia Pacific Ltd** having their offices at L43, Office Tower, Langham Place, 8 Argyle Street, Mongkok, Kowloon, Hong Kong.

Therefore, Olympus Medical Systems India Private Limited is authorized to undertake/execute any decision towards sales/service activities in India.

Thanking You,  
Olympus Corporation

Authorized Signatory

  
Rie Nakase  
General Manager  
Asia-Pacific Sales Marketing Department  
Marketing Division

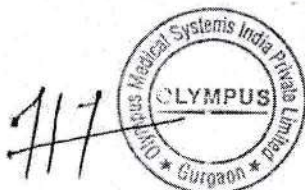

# OLYMPUS®

Your Vision, Our Future

**OLYMPUS MEDICAL SYSTEMS INDIA PRIVATE LIMITED.**  
 Ground Floor, Tower-C, SAS Tower, The Medicity Complex,  
 Sector - 38, Gurgaon 122001, Haryana, INDIA  
 Tel. : 0124-4999191 Fax : 0124-4999190  
 Website : www.olympusmedical.co.in  
 CIN : U33110HR2009FTC039611

Ref: AIIMS/OMSI/17-18/1027

Date: 19.02.2018

To,  
 The Director  
 All India Institute of Medical Sciences,  
 Bhubaneswar, Odisha

Ref: - Offer for Upper GI Endoscope Adult against Mail Dtd 10-02-2018 regarding the purchase on PAC


## CMC -COMPREHENSIVE ANNUAL MAINTENANCE CONTRACT AFTER WARRANTY PERIOD

| YEARS                         | AMOUNT IN RS. | AMOUNT IN WORD                                         |
|-------------------------------|---------------|--------------------------------------------------------|
| Rate for 1 <sup>st</sup> year | 109650.00     | (Rupees One Lakh Nine Thousand Six Hundred Fifty only) |
| Rate for 2 <sup>nd</sup> year | 109650.00     | (Rupees One Lakh Nine Thousand Six Hundred Fifty only) |
| Rate for 3 <sup>rd</sup> year | 109650.00     | (Rupees One Lakh Nine Thousand Six Hundred Fifty only) |
| Rate for 4 <sup>th</sup> year | 109650.00     | (Rupees One Lakh Nine Thousand Six Hundred Fifty only) |
| Rate for 5 <sup>th</sup> year | 109650.00     | (Rupees One Lakh Nine Thousand Six Hundred Fifty only) |

**Note:** GST @ 18% extra as applicable. (Any change in Govt. Levies will be applied at the time of billing).

For Olympus Medical Systems India Pvt. Ltd.,

117  
 Authorised Signatory



**OLYMPUS®**

Your Vision, Our Future

**OLYMPUS MEDICAL SYSTEMS INDIA PRIVATE LIMITED.**  
Ground Floor, Tower-C, SAS Tower, The Medicity Complex,  
Sector - 38, Gurgaon 122001, Haryana, INDIA  
Tel. : 0124-4999191 Fax : 0124-4999190  
Website : www.olympusmedical.co.in  
CIN : U33110HR2009FTC039611

Dated: 19<sup>th</sup> Feb, 2018

Ref: OMSI/17-18/1036

To,  
The Director,  
ALL INDIA INSTITUTE OF MEDICAL SCIENCES,  
AIIMS Road, Patrapada,  
Bhubaneswar, (Odisha) – 751 019

Sub: Proprietary Article Certificate for Olympus High Definition VideoGastrosopes –  
Model no. : GIF-HQ190

Dear Sir,

This is to certify that “Olympus High Definition VideoGastrosopes - Model no. : Model No.- GIF-HQ190 - with DF, NBI and one touch connector” is being solely manufactured by Olympus Corporation of Asia Pacific Ltd., Japan having its manufacturing factory at Shinjuku Monolith, 3-1 Nishi-Shinjuku 2 – chome, Shinjuku-ku, Tokyo 163-0914, Japan.

This is to certify & confirm that **High Definition VideoGastrosopes - Model no. : Model No.- GIF-HQ190** is fully compatible with your existing Video Processor (Model : CV-190) & Xenon Light Source (Model CLV-190).

No other company manufactured the **High Definition VideoGastrosopes - Model no. : GIF-HQ190** which is compatible with existing Processor & Xenon Light Source.

These items are proprietary of Olympus Corporation.

Thanking you,

For Olympus Medical Systems India Pvt. Ltd.

Authorized Signatory



|   |                                                                                                                                                                                                                                                                 |  |                                                |                      |
|---|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--|------------------------------------------------|----------------------|
| 4 | Upper GI Endoscope Adult :- 01 (one)                                                                                                                                                                                                                            |  | GIF-HQ190                                      | As per specification |
|   | Field of view: Normal and Near focus 140 degree or more                                                                                                                                                                                                         |  | 140 degree                                     | As per specification |
|   | Direction of view: 0 degree, forward viewing                                                                                                                                                                                                                    |  | 0 deg                                          | As per specification |
|   | Depth of field: 2-6 mm near and 5-100 mm normal                                                                                                                                                                                                                 |  | 2-6 mm nr and 5-100 mm nor                     | As per specification |
|   | Distal end outer diameter: 9.9 mm or less                                                                                                                                                                                                                       |  | 9.9 mm                                         | As per specification |
|   | Insertion tube outer diameter: 9.9 mm or less                                                                                                                                                                                                                   |  | 9.9 mm                                         | As per specification |
|   | Tip bending range: Up 210 deg, Down 90 deg, Left & Right 100 deg.                                                                                                                                                                                               |  | Up 210 deg, Down 90 deg, Left & Right 100 deg. | As per specification |
|   | Working length: 1030 mm or more                                                                                                                                                                                                                                 |  | 1030 mm                                        | As per specification |
|   | Channel inner diameter: 2.8 mm or more                                                                                                                                                                                                                          |  | 2.8 mm                                         | As per specification |
|   | Should have HDTV compatible CCD with Near & Normal focus observation capacity                                                                                                                                                                                   |  | HDTV                                           | As per specification |
|   | Should be equipped with Auxiliary water jet for mucosal cleaning                                                                                                                                                                                                |  | Water jet available                            | As per specification |
|   | Fully immersible in disinfectant solution (no need to attach water resistant cap) & one touch connectivity.                                                                                                                                                     |  | Fully immersible                               | As per specification |
|   | The endoscope should be compatible with a processor capable of optical chromo endoscopy                                                                                                                                                                         |  | Narrow Band Imaging                            | As per specification |
|   | It should provide high resolution vision.                                                                                                                                                                                                                       |  | HDTV                                           | As per specification |
|   | It must be latest and using high-end technology                                                                                                                                                                                                                 |  | Latest & High end                              | As per specification |
|   | 0 Standard accessories Standard accessories including                                                                                                                                                                                                           |  |                                                |                      |
|   | 8 Compatible oval biopsy forceps- 5 in number                                                                                                                                                                                                                   |  | FB - 25K                                       | Standard type        |
|   | 9 Reusable alligator biopsy forceps-5 in number                                                                                                                                                                                                                 |  | FB - 25K                                       | Standard type        |
|   | 10 Cleaning brush - 5 in number                                                                                                                                                                                                                                 |  | BW-20T                                         | As per specification |
|   | 11 Extra suction and air water channel valves- 2 in number                                                                                                                                                                                                      |  | MH-443, MH-438                                 | As per specification |
|   | 12 Biopsy valve- 10 packets                                                                                                                                                                                                                                     |  | MB-358                                         | As per specification |
|   | The endoscope must be compatible with our existing light source & video processor (190 series) which are available in the Endoscopy Suite, Department of Gastroenterology, AIIMS, Bhubaneswar.                                                                  |  | Compatible                                     | As per specification |
|   | Provide with latest compact high end computer (desktop with high storage capacity at least 1 TB), with latest processor with original latest windows and fully installed original latest Microsoft office version (one time purchase & installation), antivirus |  | i5 computer, Printer, UPS (1 KVA)              | As per specification |
|   | Terms and conditions:                                                                                                                                                                                                                                           |  |                                                |                      |
|   | The system must have a standard comprehensive warranty of 5 years with spares and should quote CMC for next 5 years.                                                                                                                                            |  | Warranty 5 years                               | As per specification |
|   | It should be certified that if the instrument becomes non functional, it will be repaired within the shortest possible time period otherwise a penal charge will be levied on the company.                                                                      |  | repaired within shortest time                  | As per specification |
|   | The vender should have service centre in Bhubaneswar                                                                                                                                                                                                            |  | Local Service personnel based in Bhubaneswar   |                      |

**OLYMPUS**


Your Vision, Our Future

**EVIS EXERA III**

EVIS EXERA III GASTROINTESTINAL VIDEOSCOPE

**GIF-HQ190**

Amazing image quality for upper GI endoscopy

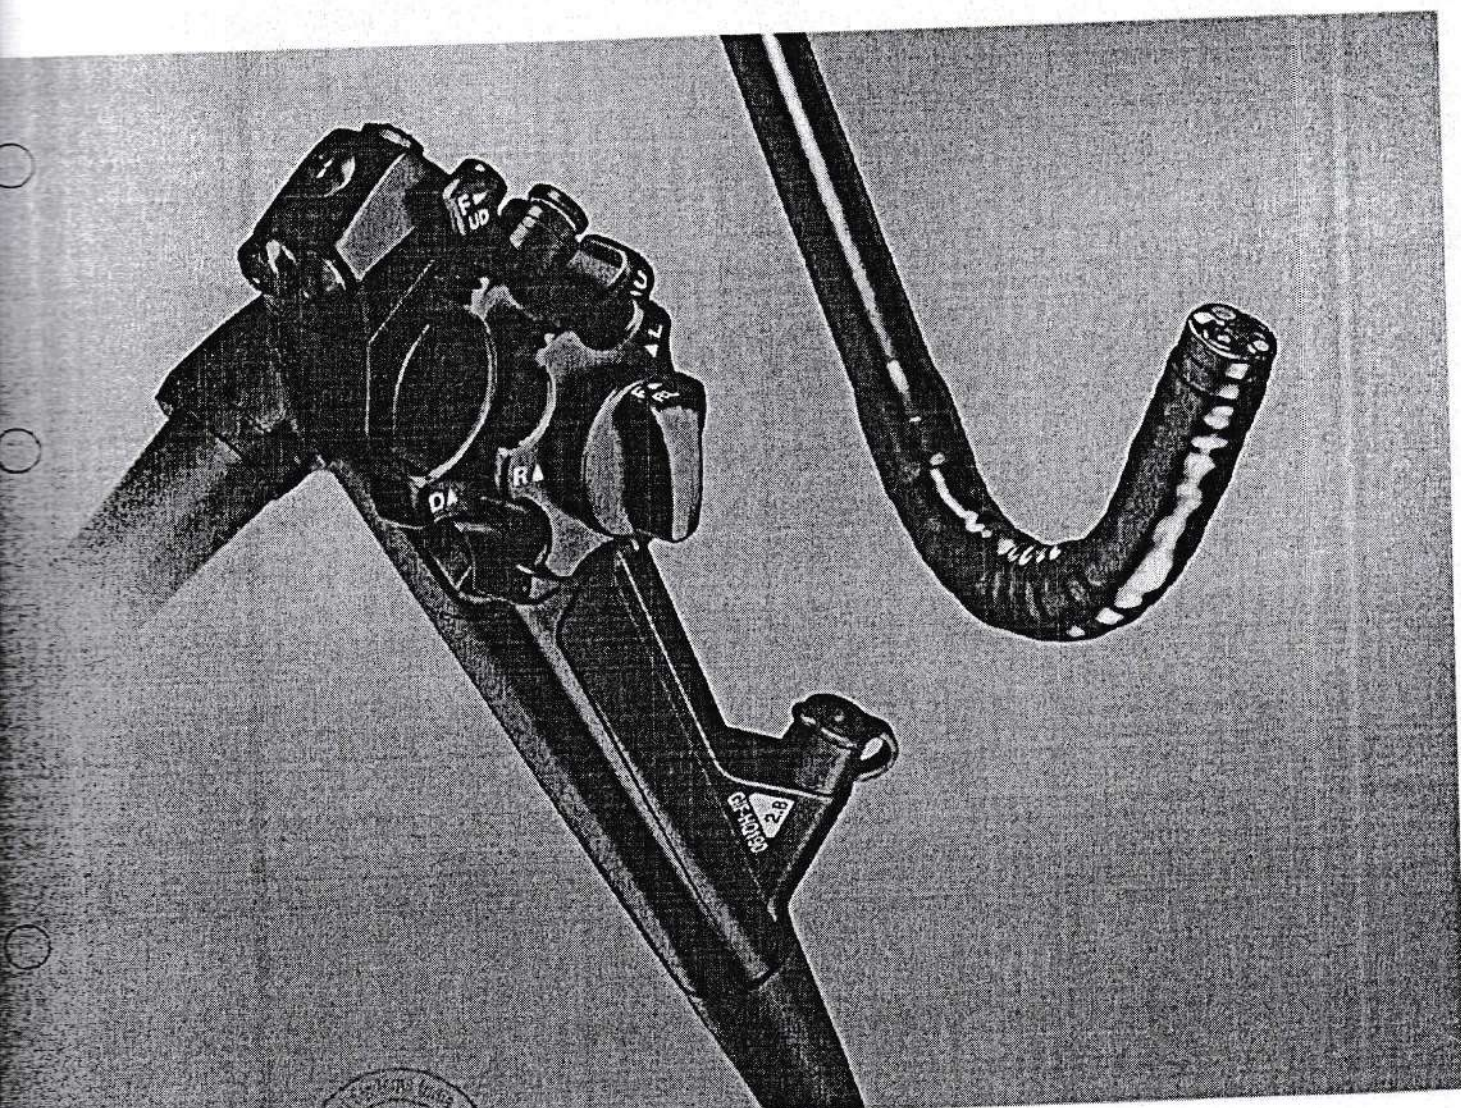

# EVIS EXERA III GASTROINTESTINAL VIDEOSCOPE OLYMPUS GIF-HQ190




## Main Features

### Dual Focus

Dual focus, a unique OLYMPUS optical innovation, allows the user to select from two focus settings. With the simple push of a scope button, the desired depth of field for observation can be optimized to either the near field or normal field.



Normal focus mode

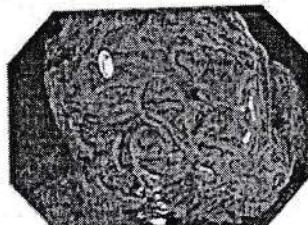


Near focus mode

### Enhanced Image Quality

A new level of resolving power is achieved thanks to a new optical system. Significantly less halation and noise is visible on screen. And the pre-freeze function automatically selects the sharpest still images.

### NBI (Narrow Band Imaging)

NBI in EVIS EXERA III 190 Series scopes provides twice the viewable distance of EVIS EXERA II 180 Series scopes and offers much greater contrast between blood vessels and mucosa. The greatly improved performance of NBI opens up exciting new clinical applications and reinforces NBI's position as the standard of care for GI endoscopy.

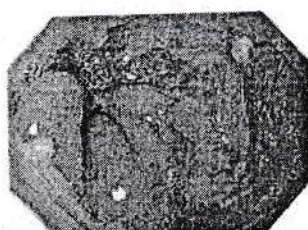


White Light



NBI

### Water Jet

EVIS EXERA III 190 Series scopes' forward water jet function is standard on all routine gastroscopes. This technology improves procedures and treatment.

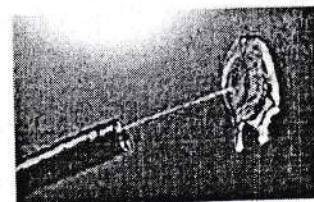

### Waterproof One-touch Connector

A new connector design minimizes the effort required for setup prior to and in between cases. In addition, it is fully submersible and eliminates the need for a water-resistant cap and the associated risk of an expensive repair due to accidental immersion.



## Specifications

|                   |                               |                                |
|-------------------|-------------------------------|--------------------------------|
| Optical System    | Field of view                 | Normal 140°<br>Near 140°       |
|                   | Direction of view             | Forward viewing                |
|                   | Depth of field                | Normal 5-100 mm<br>Near 2-6 mm |
|                   | Distal end outer diameter     | 9.9 mm                         |
| Insertion Section | Distal end enlarged           |                                |
|                   |                               |                                |
|                   | Insertion tube outer diameter | 9.9 mm                         |
|                   | Working length                | 1030 mm                        |

|                              |                                                                                  |                            |
|------------------------------|----------------------------------------------------------------------------------|----------------------------|
| Instrument Channel           | Channel inner diameter                                                           | 2.8 mm                     |
|                              | Minimum visible distance                                                         | 3.0 mm from the distal end |
|                              | Direction from which endotherapy accessories enter and exit the endoscopic image |                            |
| Bending Section              | Angulation range                                                                 | Up 210°                    |
|                              |                                                                                  | Down 90°                   |
|                              |                                                                                  | Right 100°                 |
|                              |                                                                                  | Left 100°                  |
| Total Length                 |                                                                                  | 1350 mm                    |
| Compatible EVIS EXERA System | Video System Center OLYMPUS CV-190<br>Xenon Light Source OLYMPUS CLV-190         |                            |

Dual focus image: Image courtesy of Roy Soetikno, MD  
NBI image: Image courtesy of Horst Neuhaus, MD

Specifications, design and accessories are subject to change without any notice or obligation on the part of the manufacturer.

**OLYMPUS**

OLYMPUS MEDICAL SYSTEMS CORP.  
Shinjuku Monolith, 2-3-1 Nishi-Shinjuku, Shinjuku-ku, Tokyo 163-0014, Japan

For a complete listing of sales and distribution locations visit:  
[www.olympus.com](http://www.olympus.com)

Printed in Japan G000000-0000



## ANNEXURE-VIII

**OLYMPUS®**

Your Vision, Our Future

**OLYMPUS MEDICAL SYSTEMS INDIA PRIVATE LIMITED.**  
 Ground Floor, Tower-C, SAS Tower, The Medicity Complex,  
 Sector - 38, Gurgaon 122001, Haryana, INDIA  
 Tel. : 0124-4999191 Fax : 0124-4999190  
 Website : www.olympusmedical.co.in  
 CIN : U33110HR2009FTC039611

Date : 19.02.2018

Ref: AIIMS/OMSI/17-18/1027

To,  
 The Director  
 All India Institute of Medical Sciences,  
 Bhubaneswar, Odisha

Ref: - Offer for Upper GI Endoscope Adult against Mail Dtd 10-02-2018 regarding the purchase on PAC

| MATERIAL                        | HSN CODE | PART CODE                     | DESCRIPTIONS                                              | QTY.               | PRICE (INR) | GST | FINAL PRICE INCL GST |
|---------------------------------|----------|-------------------------------|-----------------------------------------------------------|--------------------|-------------|-----|----------------------|
| <b>Upper GI Endoscope Adult</b> |          |                               |                                                           |                    |             |     |                      |
| N3802930                        | 9018     | GIF-HQ190 W/BR (EN)           | GIF TYPE HQ190 EVIS EXERA III GASTROINTESTINAL VIDEOSCOPE | 1                  | 2050081     | 12% | 2296091              |
| <b>Consisting of</b>            |          |                               |                                                           |                    |             |     |                      |
| 4802330                         | 9018     | FB-25K-1                      | FB-25K-1 BIOPSY FORCEPS (FENESTRATED)                     | 5                  | 75840       | 12% | 84941                |
| 4802330                         | 9018     | FB-25K-1                      | FB-25K-1 BIOPSY FORCEPS (FENESTRATED)                     | 5                  | 75840       | 12% | 84941                |
| GV803800                        | 9018     | BW-20T CHANNEL CLEANING BRUSH | BW-20T CHANNEL CLEANING BRUSH                             | 5                  | 20854       | 12% | 23356                |
| GV394900                        | 8481     | MH-443                        | SUCTION VALVE                                             | 2                  | 7817        | 18% | 9224                 |
| GV404200                        | 8481     | MH-438                        | A/W VALVE                                                 | 2                  | 9142        | 18% | 10787                |
| GX0283                          | 8481     | MB-358                        | BIOPSY VALVE                                              | 10 Pkt             | 14694       | 18% | 17338                |
| A10000000520                    |          | COMPUTER SYSTEM               | COMPUTER IS PROCESSOR WITH ANTI VIRUS                     | 1                  | 65071       | 18% | 76783                |
| A10000000530                    |          | PRINTER                       | COLOR LASERJET PRINTER                                    | 1                  | 20334       | 18% | 23994                |
| A10000000490                    |          | UPS                           | 2KVA UPS                                                  | 1                  | 57497       | 18% | 67846                |
|                                 |          |                               |                                                           | <b>TOTAL PRICE</b> |             |     | <b>2695303</b>       |

RUPEES TWENTY SIX LAKH NINETY FIVE THOUSAND THREE HUNDRED THREE ONLY

**TERMS & CONDITIONS :**

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                |
|--------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Price              | Price quoted is FOR destination Hospital Site.                                                                                                                                                                                                                                                                                                                                                                 |
| Local Taxes        | Included (Any change in Govt. Levies will be applied at the time of billing).                                                                                                                                                                                                                                                                                                                                  |
| Octroi/Entry Taxes | Extra & to be borne by the customer                                                                                                                                                                                                                                                                                                                                                                            |
| Way Bill           | Way Bill wherever applicable has to be provided by the customer before dispatch of material.                                                                                                                                                                                                                                                                                                                   |
| Order Placement    | Order is to be placed in favour of: M/S Olympus Medical Systems India Pvt. Ltd., having office at Plot No. 536, GF Udyog Vihar, Phase - V, Gurgaon - 122001, India                                                                                                                                                                                                                                             |
| Payment Terms      | As per AIIMS Terms and Conditions                                                                                                                                                                                                                                                                                                                                                                              |
| Delivery           | As per AIIMS Terms and Conditions                                                                                                                                                                                                                                                                                                                                                                              |
| Warranty           | We warrant the equipment against manufacturing defects, if any for a period of 60 months from the date of installation or 61 months from the date of invoice to the customer whichever is earlier.<br>This warranty does not cover consumables, Accessories, normal wear, & tear, wrongful handling, not following the user instructions given in the literature and unauthorized attachments or modifications |
| Validity           | As per AIIMS Terms and Conditions                                                                                                                                                                                                                                                                                                                                                                              |

For Olympus Medical Systems India Pvt. Ltd.


 Authorised Signatory